



Australian Government
**National Measurement
Institute**

Bradfield Road, West Lindfield NSW 2070

Cancellation
Certificate of Approval No 6/4C/229

Issued by the Chief Metrologist under Regulation 60
of the
National Measurement Regulations 1999

This is to certify that the approval for use for trade granted in respect of the

NCR Model 7876-2000 Weighing Instrument

submitted by NCR Corporation
 2651 Satellite Blvd
 Duluth Georgia 30096
 USA

has been cancelled in respect of new instruments as from 1 December 2010.

Signed by a person authorised by the Chief Metrologist
to exercise his powers under Regulation 60 of the
National Measurement Regulations 1999.

A handwritten signature in black ink, consisting of a series of loops and flourishes, positioned to the right of the signature text.



Australian Government

**National Measurement
Institute**

12 Lyonpark Road, North Ryde NSW 2113

Certificate of Approval

No 6/4C/229

Issued by the Chief Metrologist under Regulation 60
of the
National Measurement Regulations 1999

This is to certify that an approval for use for trade has been granted in respect of the
NCR Model 7876-2000 Weighing Instrument

submitted by NCR Corporation
2651 Satellite Blvd Duluth
Georgia 30096
USA.

NOTE: This Certificate relates to the suitability of the pattern of the instrument for use for trade only in respect of its metrological characteristics. This Certificate does not constitute or imply any guarantee of compliance by the manufacturer or any other person with any requirements regarding safety.

CONDITIONS OF APPROVAL

This approval becomes subject to review on 1 January 2010, and then every 5 years thereafter.

Instruments purporting to comply with this approval shall be marked with approval number 'NMI 6/4C/229' and only by persons authorised by the submitter.

It is the submitter's responsibility to ensure that all instruments marked with this approval number are constructed as described in the documentation lodged with the National Measurement Institute (NMI) and with the relevant Certificate of Approval and Technical Schedule. Failure to comply with this Condition may attract penalties under Section 19B of the National Measurement Act and may result in cancellation or withdrawal of the approval, in accordance with document NMI P 106.

The National Measurement Institute reserves the right to examine any instrument or component of an instrument purporting to comply with this approval.

Auxiliary devices used with this instrument shall comply with the requirements of General Supplementary Certificate No S1/0/A.

DESCRIPTIVE ADVICE

Pattern: approved 3 December 2004

- An NCR model 7876-2000 self-indicating weighing instrument of 13.995 kg maximum capacity.

Variants: approved 3 December 2004

1. Of 9.995 kg maximum capacity.
2. Model 7876-5000.

Technical Schedule No 6/4C/229 describes the pattern and variants 1 & 2.

FILING ADVICE

The documentation for this approval comprises:

Certificate of Approval No 6/4C/229 dated 14 January 2005
Technical Schedule No 6/4C/229 dated 14 January 2005 (incl. Test Procedure)
Figures 1 to 3 dated 14 January 2005

Signed by a person authorised by the Chief Metrologist to exercise his powers under Regulation 60 of the National Measurement Regulations 1999.

A handwritten signature in black ink, appearing to be 'J. G. T.', located at the bottom right of the page.

TECHNICAL SCHEDULE No 6/4C/229

Pattern: NCR Model 7876-2000 Weighing Instrument

Submittor: NCR Corporation
2651 Satellite Blvd
Duluth Georgia 30096 USA

1. Description of Pattern

An NCR model 7876-2000 (#1) self-indicating weighing instrument (Figure 1) of 13.995 kg maximum capacity with a verification scale interval of 0.005 kg.

Instruments may be fitted with output sockets (output interfacing capability) for the connection of auxiliary and/or peripheral devices.

Instruments are fitted with one or two model 7825 (#2) displays mounted on a column (Figure 2). Instruments are marked 'NOT FOR TRADING DIRECT WITH THE PUBLIC' (or similar wording) unless two displays are present or unless the single display is located such that all primary indications are clearly and simultaneously displayed to both the vendor and the customer.

Instruments may be fitted with an extended weighing platform attachment ('produce guard') as shown in Figure 3 (#1).

Instruments are approved for use over a temperature range of +10°C to +40°C and must be so marked.

Instruments use an AcBel model API-8545 power supply; the submitter should be consulted regarding the acceptability of alternatives.

Instruments are provided with an integral laser scanner for reading bar codes.

(#1) The last three digits of the model number (7876-2****) may be numerals other than '0', but these represent features which are not metrologically significant.

(#2) May also be marked as 'Class 7825'.

1.1 Zero

Zero is automatically corrected to within $\pm 0.25e$ whenever power is applied and whenever the instrument comes to rest within $0.5e$ of zero.

The initial zero-setting device of the pattern has a nominal range of not more than 20% of the maximum capacity of the instrument.

The instrument has a semi-automatic zero-setting device with a nominal range of not more than 4% of the maximum capacity of the instrument.

1.2 Display Check

A display check is initiated whenever power is applied.

1.3 Scanner

Instruments are provided with an integral laser scanner for reading bar codes.

1.4 Verification/Certification Provision

Provision is made for the application of a verification/certification mark.

1.5 Sealing Provision

Provision is made for the calibration adjustments to be sealed by means of a cover over the calibration adjustment switch located under the load receptor – the cover may be sealed by means of a destructible adhesive label or by a lead and wire type seal.

1.6 Markings

Instruments carry the following markings:

Manufacturer's mark, or name written in full	NCR Corporation
Name or mark of manufacturer's agent
Indication of accuracy class	Ⓜ
Maximum capacity	<i>Max</i> kg *
Minimum capacity	<i>Min</i> kg *
Verification scale interval	<i>e</i> = kg *
Serial number of the instrument
Pattern approval mark for the indicator	NMI 6/4C/229
Special temperature limits	+10°C to +40°C

* These markings are also shown near the display of the result if they are not already located there.

2. Description of Variants

2.1 Variant 1

A model 7876-2000 weighing instrument of 9.995 kg maximum capacity with a verification scale interval of 0.005 kg.

2.2 Variant 2

A model 7876-5000 (#) weighing instrument of either 9.995 kg maximum capacity or 13.995 kg maximum capacity with a verification scale interval of 0.005 kg.

This model has a smaller weigh platform than the model 7876-2000.

(#) The last three digits of the model number (7876-5***) may be numerals other than '0', but these represent features which are not metrologically significant.

TEST PROCEDURE

Instruments should be tested in accordance with any relevant tests specified in the Uniform Test Procedures.

Maximum Permissible Errors at Verification/Certification

The maximum permissible errors for increasing and decreasing loads on initial verification/certification for loads, m , expressed in verification scale intervals, e , are:

- $\pm 0.5 e$ for loads $0 \leq m \leq 500$;
- $\pm 1.0 e$ for loads $500 < m \leq 2\,000$; and
- $\pm 1.5 e$ for loads $2\,000 < m \leq 10\,000$.

Ensure that instruments are only being used within the special temperature limits stated elsewhere in this Technical Schedule.

6/4C/229
14 January 2005

FIGURE 6/4C/229 – 1



NCR Model 7876-2000 Weighing Instrument (With Two Displays
and Without Produce Guard)


6/4C/229
14 January 2005

FIGURE 6/4C/229 – 2



Typical Single Model 7825 Display

FIGURE 6/4C/229 – 3

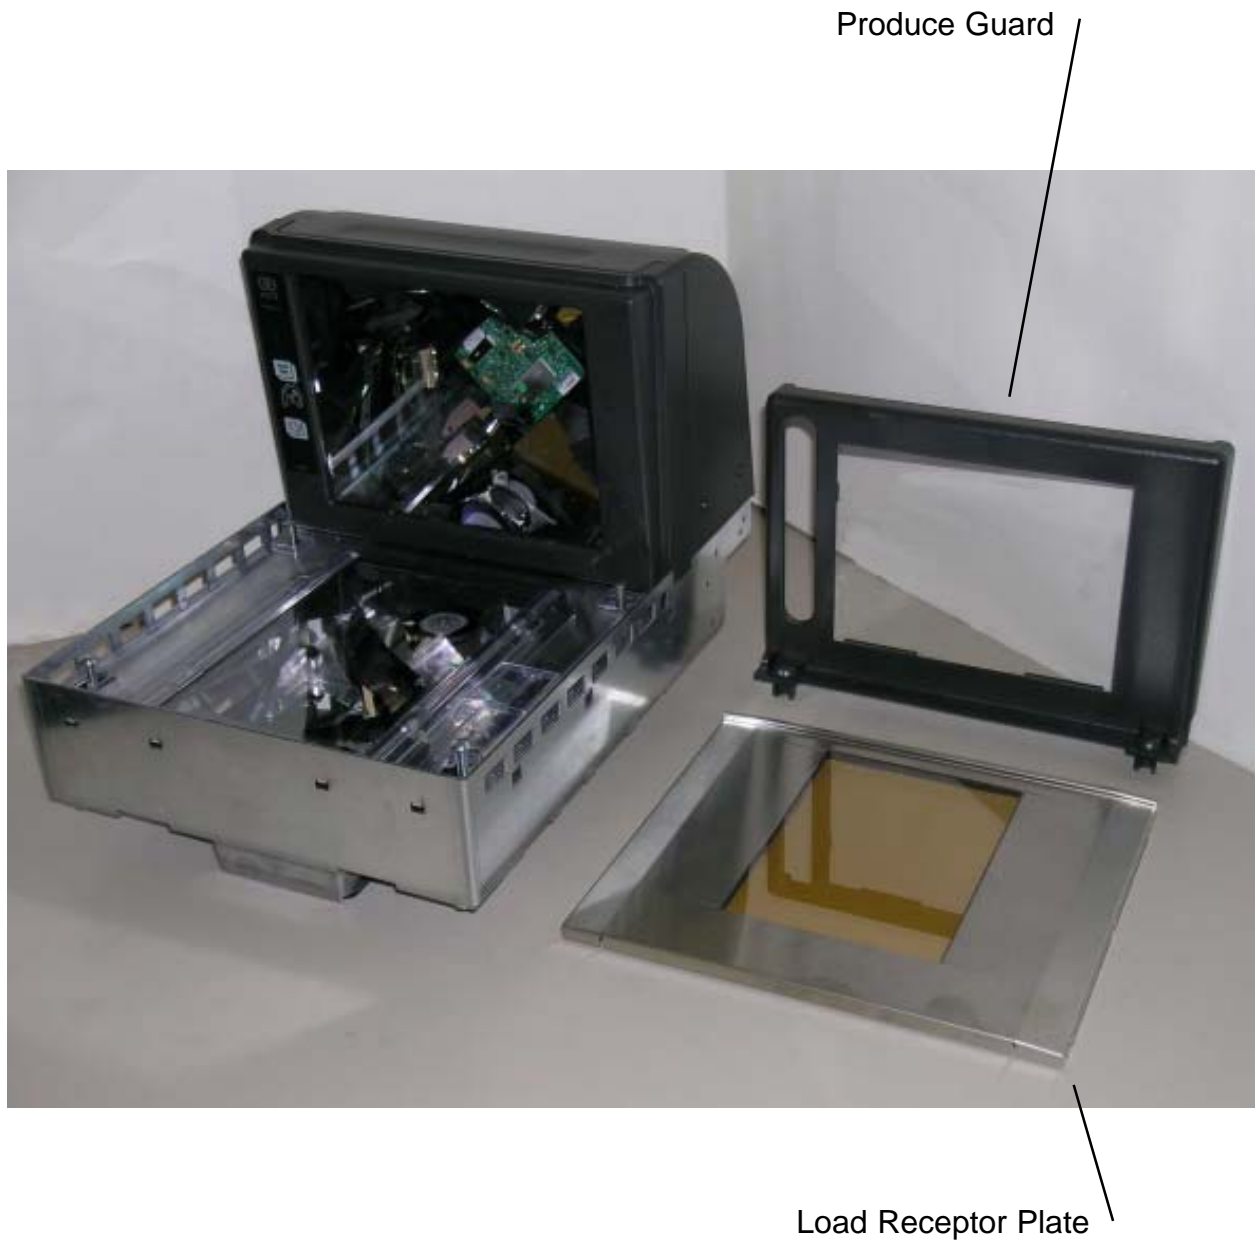

NCR Model 7876-2000 Weighing Instrument With Produce Guard and
Load Receptor Plate Removed